

# Ultraflex™

Esophageal NG Stent System

Boston  
Scientific



### Place your Trust in the Ultraflex Esophageal NG Stent System.

The Ultraflex Esophageal NG Stent System features Nitinol construction for flexibility and patient comfort and markers for enhanced visualization. Proximal and distal release delivery systems provide users with two deployment options to treat a variety of strictures throughout the esophagus and facilitate accurate stent placement.




**Distal Release**



**Proximal Release**

#### DELIVERY SYSTEM

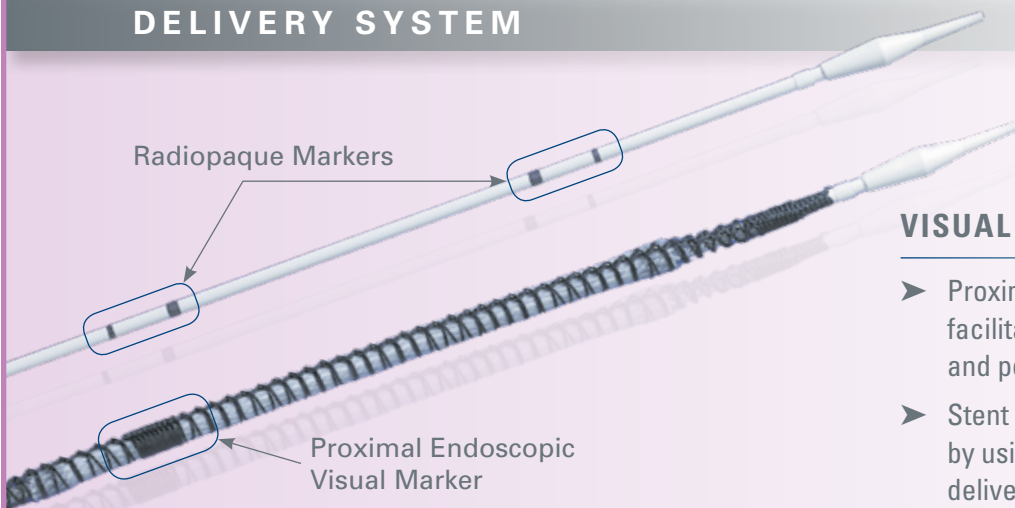

#### VISUAL MARKERS

- Proximal visual marker is designed to facilitate accurate endoscopic placement and positioning
- Stent may be placed without fluoroscopy by using the ruler on the shaft of the delivery system

## Construction

- Knitted single-strand Nitinol wire is designed to maintain luminal patency while reducing the risk of migration
- Elongated proximal flare is designed to improve fixation and reduce the incidence of food entrapment
- Flexible stent is designed to perform with peristaltic movement and is engineered for patient comfort


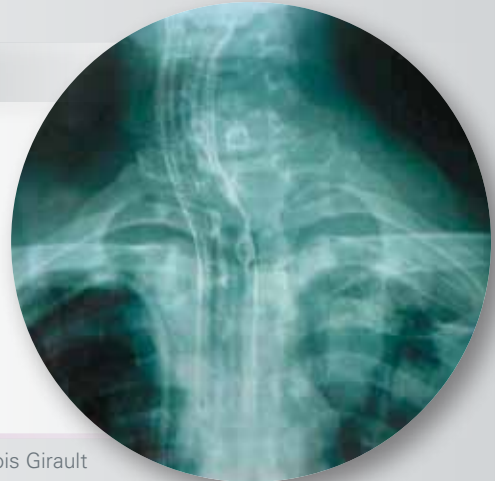


Image courtesy of Dr. Francois Girault  
Clinique du Trocadero, Paris, France.

## Suture Design

- Highly visible green sutures are engineered to facilitate endoscopic visualization of the proximal and distal ends of the stent
- Sutured looped ends are designed for stent repositioning during initial placement

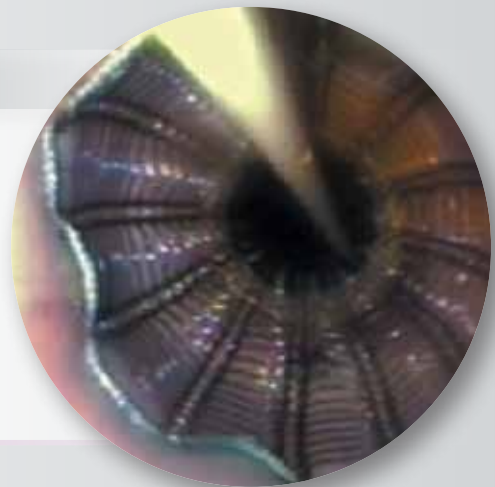

## Radial Force

- Self-radial expansion and radial compression helps the stent perform with peristaltic movement
- Radial force is engineered for luminal patency, palliation of malignant strictures and sealing esophageal fistulas when a covered stent is used





**Magnetic Resonance Conditional**  
Non-clinical testing has demonstrated that the Ultraflex Esophageal NG Stent System is MR Conditional. It can be scanned safely under the conditions outlined in the Directions For Use.

### ORDERING INFORMATION

#### COVERED

##### ULTRAFLEX SINGLE-USE COVERED ESOPHAGEAL NG STENT SYSTEM – DISTAL RELEASE\*

Order Number	Stent O.D. (mm)	Proximal Flare O.D. (mm)	Stent Length (cm)	Covered Length (cm)
M00513730	18	23	10	7
M00513740	18	23	12	9
M00513750	18	23	15	12
M00514200	23	28	10	7
M00514210	23	28	12	9

\*Recommended Guidewire 0.038" Jagwire™ Guidewire, Order #5662.

##### ULTRAFLEX SINGLE-USE COVERED ESOPHAGEAL NG STENT SYSTEM – PROXIMAL RELEASE\*

Order Number	Stent O.D. (mm)	Proximal Flare O.D. (mm)	Stent Length (cm)	Covered Length (cm)
M00513840	18	23	10	7
M00513850	18	23	12	9
M00513860	18	23	15	12
M00514240	23	28	10	7
M00514250	23	28	12	9

\*Recommended Guidewire 0.038" Jagwire Guidewire, Order #5662.  
Visible endoscopic proximal marker.

#### NON-COVERED

##### ULTRAFLEX SINGLE-USE NONCOVERED ESOPHAGEAL NG STENT SYSTEM – DISTAL RELEASE\*

Order Number	Stent O.D. (mm)	Proximal Flare O.D. (mm)	Stent Length (cm)
M00513700	18	23	7
M00513710	18	23	10
M00513720	18	23	15

\*Recommended Guidewire 0.038" Jagwire Guidewire, Order #5662.

##### ULTRAFLEX SINGLE-USE NONCOVERED ESOPHAGEAL NG STENT SYSTEM – PROXIMAL RELEASE\*

Order Number	Stent O.D. (mm)	Proximal Flare O.D. (mm)	Stent Length (cm)
M00513800	18	23	7
M00513810	18	23	10
M00513830	18	23	15

\*Recommended Guidewire 0.038" Jagwire Guidewire, Order #5662.

**Boston Scientific**  
Advancing science for life™

Boston Scientific Corporation  
One Boston Scientific Place  
Natick, MA 01760-1537  
[www.bostonscientific.com/endo-resources](http://www.bostonscientific.com/endo-resources)

**Ordering Information**  
**1.888.272.1001**

©2013 Boston Scientific Corporation  
or its affiliates. All rights reserved.

ENDO-175102-AA 1M August 2013